
Vanguard Laboratory
2635 Parkmont Ln
Olympia, Wa 98502
360-967-7010

# Certificate of Analysis

BPC-157 10 mg


Report To:
**Solyn LLC**

Compound: BPC-157
Amount: 10 mg
Laboratory ID: V260520-17 001
Date Reported: 6/8/2026
Lot Number: 1321

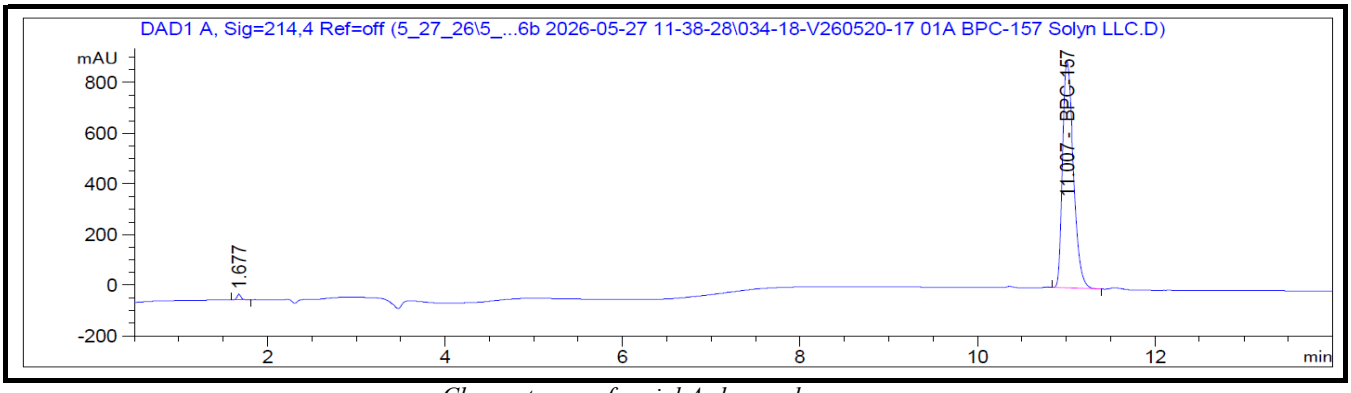


*Chromatogram for vial A shown above.*

| Analysis | Method | Result (per Vial) | | |
|---|---|---|---|---|
| Identity: Retention Time | HPLC-UV/VIS | Pass - Matches Ref. Standard | | |
| Identity: Spectral Analysis | HPLC-UV/VIS | Pass - Matches Ref. Standard | | |
| Chromatographic Purity | HPLC-UV/VIS | >99.80% | >99.80% | >99.80% |
| Assay | HPLC-UV/VIS | 10.60 mg | 10.67 mg | 10.46 mg |
| Fentanyl Screening | Immunoassay | Pass - <50 ng/mL | | |

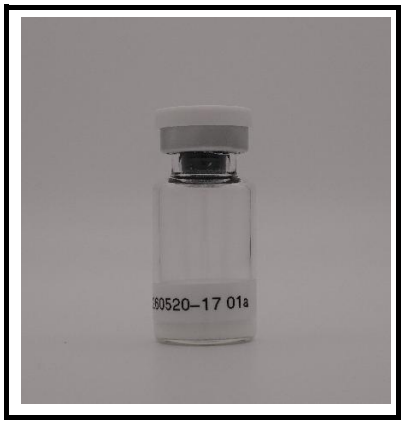


ISO 17025:2017 ACCREDITED LABORATORY

Report By: Dustin Newman, Laboratory Director on 6/8/2026

Approved By: Tori Johnson, Operations Manager on 6/8/2026

Please consult A2LA Certificate #6377.01 for a list of accredited tests. Samples were received in acceptable condition. The result(s) in this report relate only to the portion of the sample(s) tested. All analyses were performed consistent with the Vanguard Laboratory Quality Management System. Vanguard Laboratory and its staff did not observe or participate in the sample selection process, and cannot confirm the authenticity of the sample or its representativeness of the associated lot/batch.

Vanguard Laboratory
2635 Parkmont Ln
Olympia, Wa 98502
360-967-7010

# Certificate of Analysis

BPC-157 10 mg

Report To:
**Solyn LLC**

Compound: BPC-157
Amount: 10 mg
Laboratory ID: V260520-17 001
Date Reported: 6/8/2026
Lot Number: 1321

| Analyte | Method | LOQ (ppm) | Result (per Vial) | |
|---|---|---|---|---|
| Chromium (Cr) | ICP-MS | 0.05 | ND | ND |
| Arsenic (As) | ICP-MS | 0.01 | 0.01 | ND |
| Cadmium (Cd) | ICP-MS | 0.01 | ND | ND |
| Lead (Pb) | ICP-MS | 0.02 | ND | ND |
| Mercury (Hg) | ICP-MS | 0.005 | ND | ND |

Run ID: 260508

| Analysis | Method | Result (per Vial) | |
|---|---|---|---|
| Endotoxins | LAL | **A** | Pass - <5.00 EU/mg* |
| | | **B** | Pass - <5.00 EU/mg* |

*Pass/Fail criteria based on the USP/FDA threshold of 5 EU/kg (350 EU total for a 70 kg adult)

| Analysis | Method | Result (per Vial) | |
|---|---|---|---|
| Sterility | USP <71> | **A** | Pass - No Growth |
| | | **B** | Pass - No Growth |
| | | **C** | Pass - No Growth |
| | | **D** | Pass - No Growth |

Report By: Dustin Newman, Laboratory Director on 6/8/2026

Approved By: Tori Johnson, Operations Manager on 6/8/2026

*ND: Non-Detect*
*LOD: Limit of Quantification*

ISO 17025:2017 ACCREDITED LABORATORY

Please consult A2LA Certificate #6377.01 for a list of accredited tests. Samples were received in acceptable condition. The result(s) in this report relate only to the portion of the sample(s) tested. All analyses were performed consistent with the Vanguard Laboratory Quality Management System. Vanguard Laboratory and its staff did not observe or participate in the sample selection process, and cannot confirm the authenticity of the sample or its representativeness of the associated lot/batch.

Vanguard Laboratory
2635 Parkmont Ln
Olympia, Wa 98502
360-967-7010

# Certificate of Analysis

BPC-157 10 mg

Report To:
**Solyn LLC**

Compound: BPC-157
Amount: 10 mg
Laboratory ID: V260520-17 001
Date Reported: 6/8/2026
Lot Number: 1321

| Residual Solvents Analysis | | | |
|---|---|---|---|
| **Analyte** | **Method** | **LOQ (ppm)** | **Result (ppm)** |
| Acetone | GC-MS | 3.7 | ND |
| Benzene | GC-MS | 0.02 | ND |
| Butanes | GC-MS | 3.7 | ND |
| Chloroform | GC-MS | 0.02 | ND |
| Cyclohexane | GC-MS | 2.9 | ND |
| Dichloromethane | GC-MS | 0.45 | ND |
| Ethanol | GC-MS | 3.7 | ND |
| Ethyl Acetate | GC-MS | 3.7 | ND |
| Heptane | GC-MS | 3.7 | ND |
| Hexanes | GC-MS | 0.21 | ND |
| Isopropanol | GC-MS | 3.7 | ND |
| Methanol | GC-MS | 2.2 | ND |
| Pentanes | GC-MS | 3.7 | ND |
| Propane | GC-MS | 3.7 | ND |
| Toluene | GC-MS | 0.66 | ND |
| Total Xylenes | GC-MS | 1.6 | ND |

| Analysis | Method | Result (per Vial) | |
|---|---|---|---|
| Container Closure Integrity | Dye Ingress Method | **A** | Pass |
| | | **B** | Pass |
| Solubility Analysis | Fully Soluble in 2 mL Water | **A** | Pass |
| Trifluoroacetic Acid (TFA) | Ion Chromotography | ND - <0.10% | |

Report By: Dustin Newman, Laboratory Director on 6/8/2026

Approved By: Tori Johnson, Operations Manager on 6/8/2026

*ND: Non-Detect*
*LOD: Limit of Quantification*

ISO 17025:2017 ACCREDITED LABORATORY

Please consult A2LA Certificate #6377.01 for a list of accredited tests. Samples were received in acceptable condition. The result(s) in this report relate only to the portion of the sample(s) tested. All analyses were performed consistent with the Vanguard Laboratory Quality Management System. Vanguard Laboratory and its staff did not observe or participate in the sample selection process, and cannot confirm the authenticity of the sample or its representativeness of the associated lot/batch.